

8-Channel Measuring Amplifier BX8



Operating manual

Released June 21, 2023

15-247 Rev B

Table of contents

| | |
|---|----|
| Measuring amplifier BX8 | 4 |
| Description | 5 |
| Versions..... | 5 |
| Interfaces..... | 5 |
| Software | 6 |
| Features | 6 |
| Signal flow | 7 |
| Galvanic isolation..... | 7 |
| Dimensions | 8 |
| BX8-HD15 | 8 |
| BX8-HD44 | 8 |
| BX8-AS | 9 |
| Specifications..... | 10 |
| Analog input..... | 10 |
| Digital input / digital output..... | 11 |
| Analog output | 11 |
| Voltage source | 11 |
| Supply | 11 |
| Environmental data | 11 |
| Interfaces | 12 |
| Resolution of strain gage input | 12 |
| Noise Amplitude at Analog Output | 12 |
| Digital filters..... | 13 |
| Finite Impulse response Filter | 13 |
| Infinite Impulse Response Filter | 13 |
| Buttons and indicators..... | 14 |
| Pin Configuration | 15 |
| Input 15-pin D-Sub HD..... | 15 |
| Input 44-pin D-Sub HD | 16 |
| Input M16 Binder 423..... | 24 |
| Connection strain gage quarter bridge | 25 |
| Connection strain gage half bridge | 26 |
| Connection strain gage full bridge..... | 26 |
| Connection of PT1000 | 27 |
| Connection of thermocouple type-K | 27 |
| Connection of the active sensors | 27 |
| Connection of the TEDS cables for sensors with Transducer Elec. Data sheet..... | 27 |
| Analog output 25-pin D-Sub socket..... | 28 |

Digital in- and outputs 25-pin D-Sub plug connector.....29
 EtherCat M12 4-pin socket D-coded.....30

CANbus M12 5-pin socket / plug A-coded..... 30
 UART Port Sub-D9 socket31
 Voltage supply M8, 4-pin.....31
 Screw terminal BX8-AS32

Additional information.....34
 LED indicators34
 LED indicators STATUS and FUNCTION on Ethercat devices.....34
 LED-display for error condition (all device models)35
 FUNCTION LED35
 STATUS LED (red).....36
 Digital inputs and outputs.....36
 Digital-I/O Numbers.....37
 Digital I/O Functions.....38
 Inverting digital inputs.....40
 Further Notes Digital I/O40
 Master-Slave Frame Synchronization.....41
 Counter, frequency, and speed measurement41

Data acquisition and Bandwidth.....42
 Data frames and data throughput.....44

Analog outputs.....46
 Transducer Electronic Data Sheet according to IEEE1451.4 (TEDS).....46
 Frequency output 60kHz \pm 30kHz (devices option).....46

Warranty47

Measuring amplifier BX8

8-channel measuring amplifier

Additionally: 2x Counter/Frequency Encoder channels 8x

analog input configurable

full, half, quarter bridges, 120- 350- 1000 Ohm, PT1000, Type K, $\pm 10V$ Outputs 1x USB Port,

8x analog output $\pm 10V$, 4...20mA configurable, 1x UART,

alternatively, EtherCat, CANbus/CANopen 16x Digital in-

and output

5x Galvanic isolation: analog-input, analog-output, digital-I/O, UART, USB 8x

48kS/s Simultaneous sampling

6-wire technology, bridge supply 2.5V, 5.0V, 8.75V configurable

Automatic configuration of analog and digital filters by specifying the data frequency

Additional Digital Filters IIR 4th order and FIR 14th order individually configurable

Resolution < 20 nV/V

1-axis, 3- and 6-axis sensors connectible

Autonomous calculation of 3 forces and moments of six-axis sensors Two
operating hours counters

Sensors with TEDS supported (readable and writeable) Integration of a
Raspberry PI in the housing cover of the BX8-AS Compatible free
software, convenient and extensive



Figure 1: BX8-HD front side



Figure 2: BX8-HD back side



Figure 3: BX8-AS



Description

This 8-channel measuring amplifier amplifies and digitizes analog signals of various sensors, e.g., passive ones with Wheatstone bridge, such as force or torque sensors, strain gages (strain gage, full- half-quarter bridge), active sensors and temperature sensors. Digital position sensors are also supported.¹

The BX8 is characterized by a high resolution at data frequencies from 1 Hz to 48000 Hz. The 8 input channels are recorded simultaneously, without multiplexing.

Versions

| Type | Sensor Input | Signal-Output |
|--------------|------------------------------|---------------------------------------|
| BX8-HD15 | 8 x 15-pin HD D-Sub | 1xUSB, UART, analog, Digital-I/O |
| BX8-HD15-EC | 8 x 15-pin HD D-Sub | 1xUSB, EtherCat, analog, Digital-I/O |
| BX8-HD15-CAN | 8 x 15-pin HD D-Sub | 1xUSB, UART, CAN, analog, Digital-I/O |
| BX8-HD44 | 4 x 44-pin HD D-Sub | 1xUSB, UART, analog, Digital-I/O |
| BX8-HD44-EC | 4 x 44-pin HD D-Sub | 1xUSB, EtherCat, analog, Digital-I/O |
| BX8-HD44-CAN | 4 x 44-pin HD D-Sub | 1xUSB, UART, CAN, analog, Digital-I/O |
| BX8-AS | 1x 24pin M16, screw terminal | 1xUSB, UART, analog, Digital-I/O |
| BX8-AS-EC | 1x 24pin M16, screw terminal | 1xUSB, EtherCat, analog, Digital-I/O |
| BX8-AS-CAN | 1x 24pin M16, screw terminal | 1xUSB, UART, CAN, analog, Digital-I/O |
| BX8-AS-PI-3 | 1x 24pin M16, screw terminal | like BX8-AS, but with Raspberry PI |

Interfaces

Communication interfaces such as USB port or EtherCAT or CANbus are available. The device has 8 configurable analog outputs (± 10 V and 4...20 mA among others). UART interface may be used to control the measuring amplifier via the Raspberry PI (not for versions with EtherCat).

The interface protocol of USB and UART is identical and described in a separate documentation (ba-BX8com.pdf). The fieldbus protocols EtherCAT and CANopen are

¹ From firmware version 1.45 on

standardized in the lower protocol layers and the application layer is described in separate documents (ba-BX8canopen.pdf and ba-BX8ethernet_en.pdf).

Software

The Windows programs BlueDAQ with graphical user interface and the console terminal program BX8terminal are suitable. A Windows function library (MEGSV8w32.dll) with commented C header is available for self-programming users and a LabView library with wrapper VIs for this DLL for programming with LabView ©.

Features

There are 8 analog inputs available. They are individually configurable as:

- Strain gage input for full bridges in 4 and 6 wire technology or
- Strain gage input for half bridges or
- Strain gage input for quarter bridges 120 ohm, 350 ohm, 1 kOhm or
- Single-ended input ± 10 V or
- Input for PT1000 temperature sensor
- Input for thermocouple sensor type K²

Additionally, there are 2 digital inputs for square wave signals for counter and frequency measurements.³

The strain gage supply voltage can be switched between 8.75 V, 5.00 V and 2.5 V, assigned to input sensitivities 2 mV/V, 3.5 mV/V or 7 mV/V.

| Bridge supply voltage | Resulting input sensitivity |
|-----------------------|-----------------------------|
| 8.75 V | 2 mV/V |
| 5 V | 3,5 mV/V |
| 2.5 V | 7 mV/V |


Up to 2 additional channels can be configured for counter or frequency measurements.³, so that the BX8 then communicates data of up to 10 measuring channels. The number of channels in the measuring data frame is configurable³

The encoder signals or rectangle signals are wired to digital inputs (see p.29); up to 2 single rectangle signals or A/B outputs of up to 2 encoders can be processed. So, Frequency/speed or position/angle can be measured with suitable encoders, also simultaneously (see p. 41).

² From firmware version 1.39 on

³ From firmware version 1.45 on

Signal flow

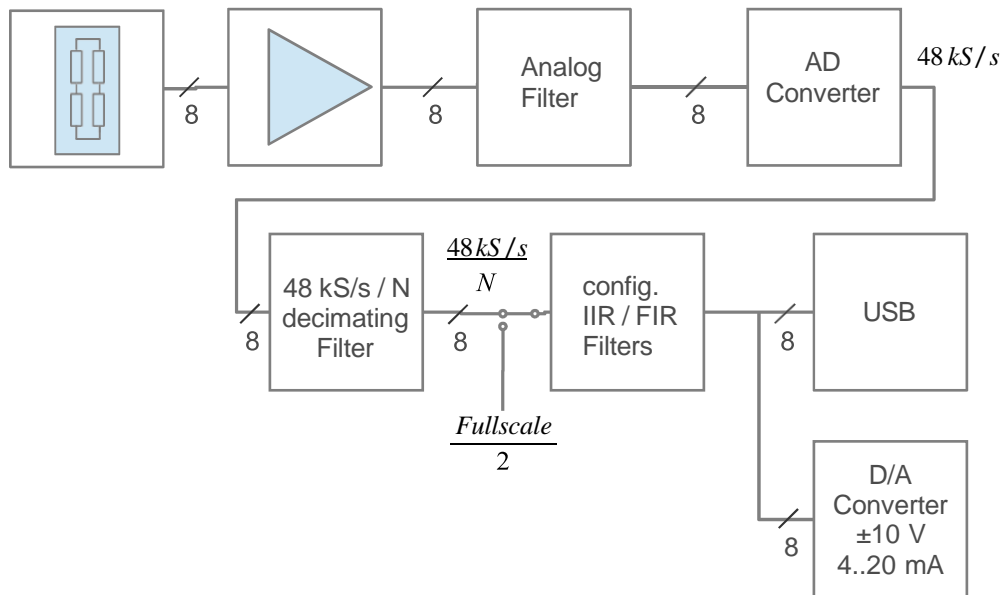

Galvanic isolation

The supply voltage UB+ / 0V is galvanically isolated from the modules for

- ✓ analog input
- ✓ analog output
- ✓ digital in- outputs
- ✓ interfaces


All these modules are also galvanically isolated from each other. The insulation voltage is 50 V. Ground lines (see table) can be connected together; the insulation doesn't apply then. Both housing types AS and DS have a ground connection, which is connected to the housing. With a high measurement data rate, it often happens that the measurement is superimposed by an external interference signal ("mains humming"). In this case, it is often helpful to connect this ground connection to a suitable ground. If the 50 or 100 Hz line noise signal is not sufficiently attenuated, you can also connect the ground of the analog input GNDE to the ground. However, this procedure eliminates the protective effect of the galvanic isolation of the analog inputs.

| | |
|-------|-------------------------------|
| UB+ | Supply voltage 12...28V DC |
| 0V | Ground Supply voltage |
| GNDE | Ground analog input |
| -Us | Negative bridge supply |
| GND A | Ground analog output |
| GND D | Ground digital input / output |


| | |
|------|---|
| GNDU | Ground UART port („Raspberry PI Port“) |
| GNDR | Ground RS232 port (V24 only as special version) |

Dimensions


BX8-HD15

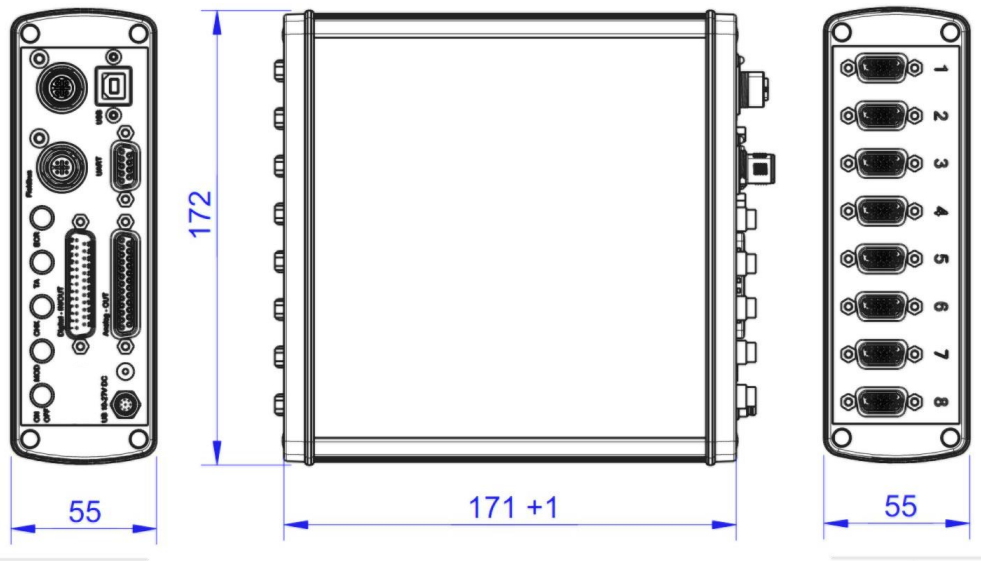

BX8-HD44

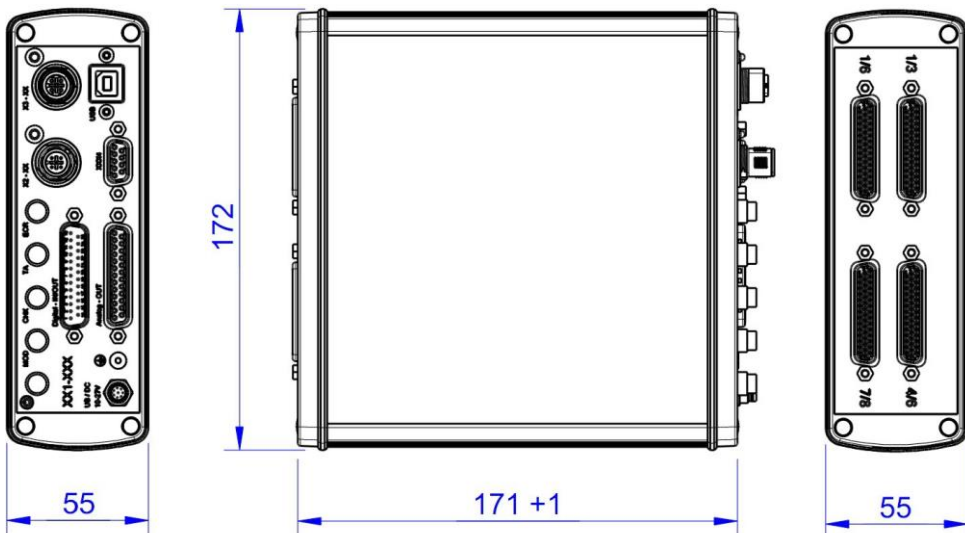

BX8-AS

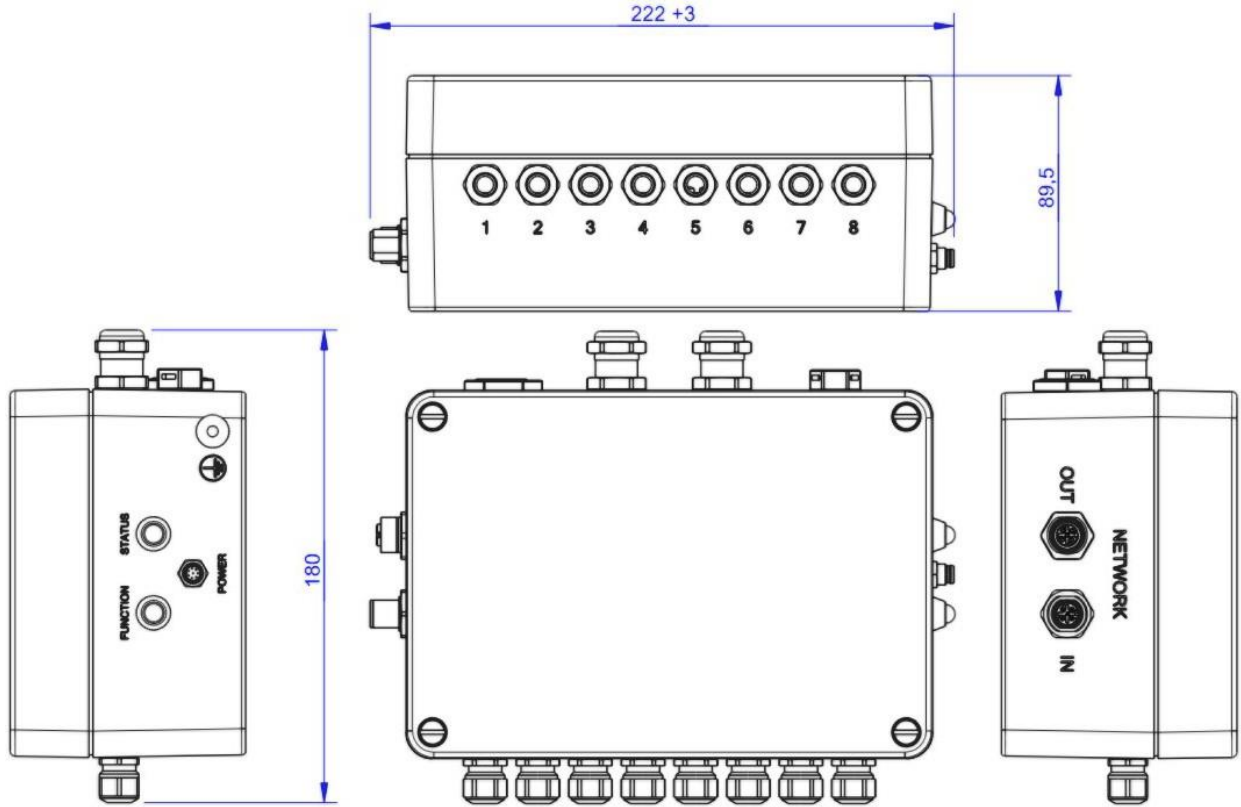

Specifications

Analog input

| | |
|---|--|
| Accuracy class | 0.05% |
| Number of analog inputs | 8 |
| Strain gage bridge input | Quarter, half, full bridge |
| Input impedance | > 20 MOhm (300pF) |
| Common mode rejection ratio DC | > 120 dB |
| Common mode rejection ratio AC 100Hz | > 100 dB |
| Strain gage bridge completions | 120 Ohm, 350 Ohm, 1 kOhm |
| Strain gage bridge supply | 2.50 V, 5.00 V, 8.75 Volt |
| Total current across all channels | 200 mA |
| Max. current per channel at bridge supply 2.5V | 40 mA (min. bridge resistance 62,5 Ohm) |
| Max. current per channel at bridge supply 5V | 60 mA (min. bridge resistance 83,3 Ohm) |
| Max. current per channel at bridge supply 8.75V | 26 mA (min. bridge resistance 336,5 Ohm) |
| Input sensitivities | 7 mV/V, 3.5 mV/V, 2 mV/V |
| Input voltage, single-ended | ±10 V |
| Input resistance | 10 MOhm |
| Input for PT1000 sensor | -230 °C ... +1500 °C |
| Excitation voltage PT1000 | 1.25 V |
| Step response delay time | 0.92 ms ⁴ |
| Delay + Settling time | 1.5 ms max ⁵ ., 1 ms typ. |

4 Measured from ±10V input to analog output, Step 0->5V, data frequency 16000/s, without additional filters

5 100% step, completely settled, worst-case

Digital input / digital output

| | |
|-----------------------------------|--|
| Number of in-/ outputs | 16 |
| Output | TTL (0V 5V), push-pull |
| total current across all channels | 140 mA |
| max. load current per output | 25 mA |
| Input | |
| max. input voltage | 5.5 V |
| min. input voltage | -0.5 V |
| Resistance Pull-up +5V | 10 kOhm |
| Sampling period | 40 msec |
| Counter / Frequency Input | |
| Measuring range counter | $\pm 8.388.608$ (internally: 32-Bit) |
| Measuring range frequency | 1/60s = 16,667 mHz to 10 MHz |
| Sampling rate | = configured data frequency 1...16000 /s |
| Supply voltage for encoders | 5V, 20mA (max) |

Analog output

| | |
|---------------------------------|--|
| Number of analog outputs | 8 |
| Configuration of analog outputs | 0...10V, -10V..+10V, 0...5V, -5V...+5V, 4...20mA |

Voltage source

| | |
|---------------------------|------------------|
| Number of voltage outputs | 8 |
| power | 8x 24V DC, 250mA |

Supply

| | |
|----------------|--------------|
| Supply voltage | 12 V to 28 V |
| Power | < 12 W |

Environmental data

| | |
|-----------------------|-----------------|
| Operating temperature | 0 °C ... +50 °C |
| Power | < 12 W |

Interfaces

| | |
|---------------|--|
| USB | 2.0 Full speed |
| Devices class | Communication Device Class, HID (firmware update only) |
| UART | Level 3.3V, galvanically isolated; auxiliary voltage 24V DC, 2A |
| EtherCat | protocol: CoE device profile 404, Mailbox- and buffered mode. Synchronization: Hardware-Latching |
| CANbus | CANopen, device profile 404, 4x TxPDOs, galvanically isolated |

Resolution of strain gage input

The resolution of measuring amplifier depends on the adjusted input sensitivity and the data frequency. The input sensitivity is assigned to the bridge supply voltage: 8.75V with 2.0 mV/V, 5V with 3.5 mV/V, 2.5V with 7 mV/V.

The excitation voltage with 8.75V is recommended only with sensors of minimum 1kOhm bridge resistance and sufficient construction size. For miniature sensors under 500g weight the bridge supply of 8.75V shall not be applied!

| | +Us | 10 Hz | 50 Hz | 100 Hz | 1 kHz | 5 kHz | 8 kHz |
|----------|--------|---------------------|---------------------|---------------------|---------------------|---------------------|---------------------|
| 3.5 mV/V | 5 V | 2.0 10 ⁵ | 1.2 10 ⁵ | 8.0 10 ⁴ | 2.5 10 ⁴ | 1.0 10 ⁴ | 8.0 10 ³ |
| 2.0 mV/V | 8.75 V | 3.0 10 ⁵ | 2.5 10 ⁵ | 1.5 10 ⁵ | 6.0 10 ⁴ | 4.0 10 ⁴ | 1.4 10 ⁴ |

At a data frequency of 10 Hz the measuring range from 0 to +3.5 is quantized in 2.0 10⁵ steps.

The noise amplitude is 17.5 nV/V.

At a sensor with rated force of 10 N and rated output of 0.5 mV/V the noise amplitude is

$$10 N \cdot \frac{0.5}{3.5} \cdot \frac{1}{2.0 \cdot 10^5} = 7.14 \cdot 10^{-6} N$$

Noise Amplitude at Analog Output

The noise amplitude at the analog output is approx. 25mV (peak values) or 10mV (RMS). It is due to the galvanic isolation of the analog output. The frequency components of the noise signal are predominantly at frequencies above 300 kHz and higher. These can be largely attenuated by the use of oversampling with subsequent digital filtering (e.g., arithmetic averaging) in the subsequent analog-digital conversion.

Digital filters

The BX8 adjusts automatically the analog filter and the „decimating“ digital input filter. The user provides only the required number of measured values per second (data frequency), which is send via USB-interface or made available to the field bus. Additionally, there are two adjustable digital filters: 1x FIR filter and 1x IIR filter. Each of these filters is individually adjustable for any of the 8 input channels. In the measured data signal processing chain, the FIR filter is processed first, followed by the IIR filter.

Finite Impulse response Filter

The FIR filter is a low pass filter with which the filter order N and the cut-off frequency fg can be set. The cut-off frequency is the frequency at which the signal is already attenuated by -3 dB. This corresponds to a factor of approx. 0.7. Frequencies lying above this will continue to be attenuated. The filter order determines the maximum and minimum adjustable cut-off frequency fg in terms of the data rate Fa, and the steepness of the attenuation range. Higher orders have a steeper slope, i.e., an increase in the signal frequency causes the attenuation to increase faster. The so-called step response is slower at higher orders however, i.e., it always takes N+1 measured values until the filter’s output value corresponds to the input value.

| Order | fg/Fa min in Hz | fg/Fa min in Hz |
|-------|-----------------|-----------------|
| 14 | 0,05 | 0,190 |
| 12 | 0,06 | 0,225 |
| 10 | 0,07 | 0,270 |
| 8 | 0,09 | 0,340 |
| 6 | 0,12 | 0,350 |
| 4 | 0,18 | 0,410 |

Infinite Impulse Response Filter

The infinite Impulse Response Filter (IIR) of fourth order allows four different filter types:

- 1) Low pass filter: Sensor signals at low frequency (including DC size with f=0) pass through the filter, signals at a higher frequency are attenuated.
- 2) High pass filter: Sensor signals at low frequency (including DC size with f=0) are attenuated, signals at a higher frequency pass through the filter. Note: Frequencies above half of the measured data rate cannot be processed. The measuring amplifier includes an analog-to-digital sampling system, which acts as a low pass.
- 3) Band pass filter: Signals are allowed to pass through within a frequency range, signals which are above or below this range are attenuated.
- 4) Band stop filter (‘Notch filter’): Signals are attenuated within a frequency range, signals which are above or below this range are allowed to pass through.

The cut-off frequency can be configured for low and high pass filters. The cut-off frequency is the frequency at which the signal is already attenuated by -3 dB. This corresponds to a factor of approx. 0.7. Frequencies lying above for low pass and lying below for high pass will continue to be attenuated.

Two cut-off frequencies can be configured for band pass and band stop filters; the upper and the lower. Attenuation by -3 dB also occurs here. The two cut-off frequencies may not be the same. Signal frequencies lying between these are allowed to pass through for the band pass filter and are attenuated for the band stop filter.

The maximum (and the minimum if need be) of each cut-off frequency is dependent on the measured data rate. Cut-off frequencies can be set to $(0.49 * \text{measured data rate})$, i.e. almost to half.


The filters can be individually configured for each channel and also switched on and off. The configuration also remains the same for filters that have been switched off.

Buttons and indicators

| | |
|--------------------------------|---|
| Power-button with LED function | Switch on and off the device (only BX8-HD) Function LED |
| Mod-button with Led status | a) reset the status LED; b) start the Firmware-updates, if during the Power On activates |
| CHK button with Check LED | Sensor Test; by pressing the CHK button the sensor signal for the unloaded condition is emulated on the input of the measuring amplifier; for sensors with calibration matrix the documented zero signals of the sensor are emulated on the inputs. |
| TA | „Tara“, Set-Zero“: trigger an automatic zero adjustment for all outputs (analog and digital) |
| ECR-LED | EtherCat EC Run; |

Pin Configuration


Input 15-pin D-Sub



Connection of strain gages, active sensors, temperature sensors and TEDS. Activation of the bridge completion with external wire from “HB” (12) to -UD (10).

| No | Symbol | Description |
|--------|--------|---|
| 1 | TEDS | Transducer Electronic Data according to IEEE 1451.4 |
| 2 | -Us | Negative bridge supply |
| 3 | +Us | Positive bridge supply |
| 4 | Q350 | Quarter bridge completion 350 Ohm |
| 5 | +UD | Positive differential input |
| 6 | GNDE | Ground, analog input |
| 7 | -Uf | Negative sense line (6-wire connection only) |
| 8 | +Uf | Positive sense line (6-wire connection only) |
| 9 | Q120 | Quarter bridge completion 120 Ohm |
| 10 | -UD | Negative differential input |
| 11 | Q1k | Quarter bridge completion 1000 Ohm |
| 12 | HB | Half bridge completion |
| 13 | VCCIO | Voltage source 24V DC, 250mA |
| 14 | Ue | analog input voltage, single ended $\pm 10V$ |
| 15 | GNDIO | Ground voltage source |
| Shield | PE | Earth (housing) |

Input 44-pin D-Sub

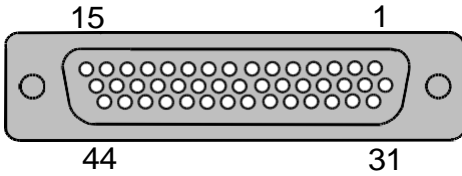

Up to 3 channels can be connected to the 44-pin D-Sub socket. The labelling on the front panel is 1/3 for connecting the channels 1 to 3.

| 1/3 Channels 1,2,3, Sub-D HD 44 | | | |
|---------------------------------|--------|--|---------|
| Pin | Signal | Description | Channel |
| Shield | PE | Earth (housing) | - |
| 1 | TEDS | Transducer Electronic Data according IEEE 1451.4 | 1 |
| 2 | US- | Negative bridge supply | 1 |
| 3 | US+ | Positive bridge supply | 1 |
| 4 | Q350 | Quarter bridge completion 350Ohm | 1 |
| 5 | UD+ | Positive differential input | 1 |
| 6 | GNDE | Ground, analog input | 1 |
| 7 | UF- | Negative sense line (6-wire connection only) | 1 |
| 8 | UF+ | Positive sense line (6-wire connection only) | 1 |
| 9 | Q120 | Quarter bridge completion 120Ohm | 1 |
| 10 | UD- | Negative differential input | 1 |
| 11 | Q1k | Quarter bridge completion 1000Ohm | 1 |
| 12 | HB | Half bridge completion | 1 |
| 13 | UE | analog input voltage, single ended $\pm 10V$ | 1 |
| 14 | GNDIO | Ground voltage source | 1 |
| 15 | PE | Earth (housing) | - |
| 16 | TEDS | Transducer Electronic Data according IEEE 1451.4 | 2 |
| 17 | US- | Negative bridge supply | 2 |
| 18 | US+ | Positive bridge supply | 2 |
| 19 | Q350 | Quarter bridge completion 350Ohm | 2 |

| | | | |
|----|------|--|---|
| 20 | UD+ | Positive differential input | 2 |
| 21 | GNDE | Ground, analog input | 2 |
| 22 | UF- | Negative sense line (6-wire connection only) | 2 |
| 23 | UF+ | Positive sense line (6-wire connection only) | 2 |
| 24 | Q120 | Quarter bridge completion 120Ohm | 2 |
| 25 | UD- | Negative differential input | 2 |
| 26 | Q1k | Quarter bridge completion 1000Ohm | 2 |
| 27 | HB | Halt bridge completion | 2 |
| 28 | UE | analog input voltage, single ended $\pm 10V$ | 2 |

| 1/3 Channels 1,2,3, Sub-D HD 44 | | | |
|---------------------------------|--------|--|---------|
| Pin | Signal | Description | Channel |
| 29 | GNDIO | Ground voltage source | 2 |
| 30 | VCCIO | Voltage source 24V DC, 250mA | 1,2,3 |
| 31 | TEDS | Transducer Electronic Data acc. to IEEE 1451.4 | 3 |
| 32 | US- | Negative bridge supply | 3 |
| 33 | US+ | Positive bridge supply | 3 |
| 34 | Q350 | Quarter bridge completion 350Ohm | 3 |
| 35 | UD+ | Positive differential input | 3 |
| 36 | GNDE | Ground, analog input | 3 |
| 37 | UF- | Negative sense line (6-wire connection only) | 3 |
| 38 | UF+ | Positive sense line (6-wire connection only) | 3 |
| 39 | Q120 | Quarter bridge completion 120Ohm | 3 |
| 40 | UD- | Negative differential input | 3 |
| 41 | Q1k | Quarter bridge completion 1000Ohm | 3 |
| 42 | HB | Half bridge completion | 3 |
| 43 | UE | analog input voltage, single ended $\pm 10V$ | 3 |
| 44 | GNDIO | Ground voltage source | 3 |

The labelling on the front panel is 4/6 for connecting the channels 4 to 6.

| 4/6 Channels 4,5,6, Sub-D HD 44 | | | |
|---------------------------------|--------|-------------|---------|
| Pin | Signal | Description | Channel |

| | | | |
|--------|------|--|---|
| Shield | PE | Earth (housing) | - |
| 1 | TEDS | Transducer Electronic Data acc. to IEEE 1451.4 | 4 |
| 2 | US- | Negative bridge supply | 4 |
| 3 | US+ | Positive bridge supply | 4 |
| 4 | Q350 | Quarter bridge completion 350Ohm | 4 |
| 5 | UD+ | Positive differential input | 4 |
| 6 | GNDE | Ground, analog input | 4 |
| 7 | UF- | Negative sense line (6-wire connection only) | 4 |
| 8 | UF+ | Positive sense line (6-wire connection only) | 4 |
| 9 | Q120 | Quarter bridge completion 120Ohm | 4 |

| 4/6 Channels 4,5,6, Sub-D HD 44 | | | |
|---------------------------------|--------|--|---------|
| Pin | Signal | Description | Channel |
| 10 | UD- | negative bridge supply | 4 |
| 11 | Q1k | Quarter bridge completion 1000Ohm | 4 |
| 12 | HB | Half bridge completion | 4 |
| 13 | UE | analog input voltage, single ended $\pm 10V$ | 4 |
| 14 | GNDIO | Ground voltage source | 4 |
| 15 | PE | Earth (housing) | - |
| 16 | TEDS | Transducer Electronic Data acc. to IEEE 1451.4 | 5 |
| 17 | US- | Negative bridge supply | 5 |
| 18 | US+ | Positive bridge supply | 5 |
| 19 | Q350 | Quarter bridge completion 350Ohm | 5 |
| 20 | UD+ | Positive differential input | 5 |
| 21 | GNDE | Ground, analog input | 5 |
| 22 | UF- | Negative sense line (6-wire connection only) | 5 |
| 23 | UF+ | Positive sense line (6-wire connection only) | 5 |
| 24 | Q120 | Quarter bridge completion 120Ohm | 5 |
| 25 | UD- | Negative differential input | 5 |
| 26 | Q1k | Quarter bridge completion 1000Ohm | 5 |
| 27 | HB | Half bridge completion | 5 |
| 28 | UE | analog input voltage, single ended $\pm 10V$ | 5 |

| | | | |
|----|-------|--|-------|
| 29 | GNDIO | Ground voltage source | 5 |
| 30 | VCCIO | Voltage source 24V DC, 250mA | 4,5,6 |
| 31 | TEDS | Transducer Electronic Data acc. to IEEE 1451.4 | 6 |
| 32 | US- | Negative bridge supply | 6 |
| 33 | US+ | Positive bridge supply | 6 |
| 34 | Q350 | Quarter bridge completion 350Ohm | 6 |
| 35 | UD+ | Positive differential input | 6 |
| 36 | GNDE | Ground, analog input | 6 |
| 37 | UF- | Negative sense line (6-wire connection only) | 6 |
| 38 | UF+ | Positive sense line (6-wire connection only) | 6 |

| 4/6 Channels 4,5,6, Sub-D HD 44 | | | |
|---------------------------------|--------|--|---------|
| Pin | Signal | Description | Channel |
| 39 | Q120 | Quarter bridge completion 120Ohm | 6 |
| 40 | UD- | Negative differential input | 6 |
| 41 | Q1k | Quarter bridge completion 1000Ohm | 6 |
| 42 | HB | Half bridge completion | 6 |
| 43 | UE | analog input voltage, single ended $\pm 10V$ | 6 |
| 44 | GNDIO | Ground voltage source | 6 |

At the 44-pin D-Sub socket 1/6 up to 6 channels can be connected. The labelling on the front panel is 1/6 for connecting the channels 1 to 6. The connections are parallel to the input jacks 1/3 and 4/6. If 1/6 is used, please leave 1/3 and 4/6 opened.

| Channels 1,2,3,4,5,6, Sub-D HD 44 | | | |
|-----------------------------------|--------|--|---------|
| Pin | Signal | Description | Channel |
| Shield | PE | Earth (housing) | - |
| 1 | UF+ | Positive sense line (6-wire connection only) | 1 |
| 2 | US+ | Positive bridge supply | 1 |
| 3 | UD+ | Positive differential input | 1 |
| 4 | UD- | Negative differential input | 1 |
| 5 | US- | Negative bridge supply | 1 |
| 6 | UF- | Negative sense line (6-wire connection only) | 1 |
| 7 | TEDS | Transducer Electronic Data according IEEE 1451.4 | 1 |
| 8 | UF+ | Positive sense line (6-wire connection only) | 2 |
| 9 | US+ | Positive bridge supply | 2 |
| 10 | UD+ | Positive differential input | 2 |
| 11 | UD- | Negative differential input | 2 |
| 12 | US- | Negative bridge supply | 2 |
| 13 | UF- | Negative sense line (6-wire connection only) | 2 |
| 14 | TEDS | Transducer Electronic Data according IEEE 1451.4 | 2 |
| 15 | PE | Earth (housing) | - |
| 16 | UF+ | Positive sense line (6-wire connection only) | 3 |
| 17 | US+ | Positive bridge supply | 3 |
| 18 | UD+ | Positive differential input | 3 |
| 19 | UD- | Negative differential input | 3 |
| 20 | US- | Negative bridge supply | 3 |
| 21 | UF- | Negative sense line (6-wire connection only) | 3 |
| 22 | TEDS | Transducer Electronic Data according IEEE 1451.4 | 3 |
| 23 | UF+ | Positive sense line (6-wire connection only) | 4 |
| 24 | US+ | Positive bridge supply | 4 |
| 25 | UD+ | Positive differential input | 4 |
| 26 | UD- | Negative differential input | 4 |
| 27 | US- | Negative bridge supply | 4 |
| 28 | UF- | Negative sense line (6-wire connection only) | 4 |


| Channels 1,2,3,4,5,6, Sub-D HD 44 | | | |
|-----------------------------------|--------|---|---------|
| Pin | Signal | Description | Channel |
| 29 | TEDS | Transducer Electronic Data acc. to IEEE 1451.4 | 4 |
| 30 | PE | Earth (housing) | - |
| 31 | UF+ | Positive sense line (6-wire connection only) | 5 |
| 32 | US+ | Positive bridge supply | 5 |
| 33 | UD+ | Positive differential input | 5 |
| 34 | UD- | Negative differential input | 5 |
| 35 | US- | Negative bridge supply | 5 |
| 36 | UF- | Negative sense line (6-wire connection only) | 5 |
| 37 | TEDS | Transducer Electronic Data according to IEEE 1451.4 | 5 |
| 38 | UF+ | Positive sense line (6-wire connection only) | 6 |
| 39 | US+ | Positive bridge supply | 6 |
| 40 | UD+ | Positive differential input | 6 |
| 41 | UD- | Negative differential input | 6 |
| 42 | US- | Negative bridge supply | 6 |
| 43 | UF- | Negative sense line (6-wire connection only) | 6 |
| 44 | TEDS | Transducer Electronic Data acc. to IEEE 1451.4 | 6 |

Note: Six-axis sensors 6A with 44-pin D-Sub connectors are connected to this socket "1/6" At the 44-pin Sub D socket 7/8 up to 2 channels can be connected (channel 7 and channel 8) .

| Channels 7, 8, Sub-D HD 44 | | | |
|----------------------------|--------|--|---------|
| Pin | Signal | Description | Channel |
| Shield | PE | Earth (housing) | - |
| 1 | UE | analog input voltage, single ended $\pm 10V$ | 1 |
| 2 | GNDE | Ground, analog input | 1 |
| 3 | UE | analog input voltage, single ended $\pm 10V$ | 2 |
| 4 | GNDE | Ground, analog input | 2 |
| 5 | UE | analog input voltage, single ended $\pm 10V$ | 3 |
| 6 | GNDE | Ground, analog input | 3 |
| 7 | UE | analog input voltage, single ended $\pm 10V$ | 4 |
| 8 | GNDE | Ground, analog input | 4 |
| 9 | UE | analog input voltage, single ended $\pm 10V$ | 5 |
| 10 | GNDE | Ground, analog input | 5 |
| 11 | UE | analog input voltage, single ended $\pm 10V$ | 6 |
| 12 | GNDE | Ground, analog input | 6 |
| 13 | PE | Earth (housing) | - |
| 14 | PE | Earth (housing) | - |
| 15 | PE | Earth (housing) | - |
| 16 | TEDS | Transducer Electronic Data according IEEE 1451.4 | 7 |
| 17 | US- | Negative bridge supply | 7 |
| 18 | US+ | Positive bridge supply | 7 |
| 19 | Q350 | Quarter bridge completion 350Ohm | 7 |
| 20 | UD+ | Positive differential input | 7 |
| 21 | GNDE | Ground, analog input | 7 |
| 22 | UF- | Negative sense line (6-wire connection only) | 7 |
| 23 | UF+ | Positive sense line (6-wire connection only) | 7 |
| 24 | Q120 | Quarter bridge completion 120Ohm | 7 |
| 25 | UD- | Negative differential input | 7 |
| 26 | Q1k | Quarter bridge completion 1000Ohm | 7 |
| 27 | HB | Half bridge completion | 7 |
| 28 | UE | analog input voltage, single ended $\pm 10V$ | 7 |

| Channels 7, 8, Sub-D HD 44 | | | |
|----------------------------|--------|--|---------|
| Pin | Signal | Description | Channel |
| 29 | GNDIO | Ground voltage source | 7 |
| 30 | VCCIO | Voltage source 24V DC, 250mA | 7,8 |
| 31 | TEDS | Transducer Electronic Data according IEEE 1451.4 | 8 |
| 32 | US- | Negative bridge supply | 8 |
| 33 | US+ | Positive bridge supply | 8 |
| 34 | Q350 | Quarter bridge completion 350Ohm | 8 |
| 35 | UD+ | Positive differential input | 8 |
| 36 | GNDE | Ground, analog input | 8 |
| 37 | UF- | Negative sense line (6-wire connection only) | 8 |
| 38 | UF+ | Positive sense line (6-wire connection only) | 8 |
| 39 | Q120 | Quarter bridge completion 120Ohm | 8 |
| 40 | UD- | Negative differential input | 8 |
| 41 | Q1k | Quarter bridge completion 1000Ohm | 8 |
| 42 | HB | Half bridge completion | 8 |
| 43 | UE | analog input voltage, single ended $\pm 10V$ | 8 |
| 44 | GNDIO | Ground voltage source | 8 |

Input M16 Binder 423

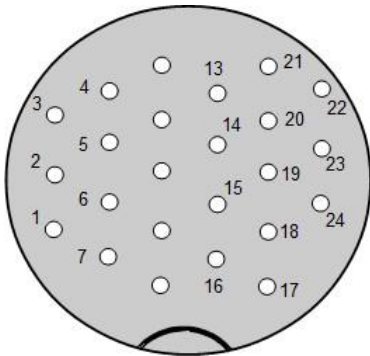


View from the plug-in side

A 6-axis sensor type 6A can be connected to the 16-pin socket of the BX8-AS.


| Channels 1,2,3,4,5,6, M16 | | | |
|---------------------------|--------|------------------------|---------|
| Pin | Signal | Description | Channel |
| Shield | PE | Housing | - |
| 1 | US+ | Positive bridge supply | 1 |
| 2 | US- | Negative bridge supply | 1 |
| 3 | UD+ | Positive bridge output | 1 |
| 4 | UD- | Negative bridge output | 1 |
| 5 | US+ | Positive bridge supply | 2 |
| 6 | US- | Negative bridge supply | 2 |
| 7 | UD+ | Positive bridge output | 2 |
| 8 | UD- | Negative bridge output | 2 |
| 9 | US+ | Positive bridge supply | 3 |
| 10 | US- | Negative bridge supply | 3 |
| 11 | UD+ | Positive bridge output | 3 |
| 12 | UD- | Negative bridge output | 3 |
| 13 | US+ | Positive bridge supply | 4 |
| 14 | US- | Negative bridge supply | 4 |
| 15 | UD+ | Positive bridge output | 4 |
| 16 | UD- | Negative bridge output | 4 |
| 17 | US+ | Positive bridge supply | 5 |
| 18 | US- | Negative bridge supply | 5 |

| Channels 1,2,3,4,5,6, M16 | | | |
|---------------------------|--------|------------------------|---------|
| Pin | Signal | Description | Channel |
| 19 | UD+ | Positive bridge output | 5 |
| 20 | UD- | Negative bridge output | 5 |
| 21 | US+ | Positive bridge supply | 6 |
| 22 | US- | Negative bridge supply | 6 |
| 23 | UD+ | Positive bridge output | 6 |
| 24 | UD- | Negative bridge output | 6 |

Connection strain gage quarter bridge

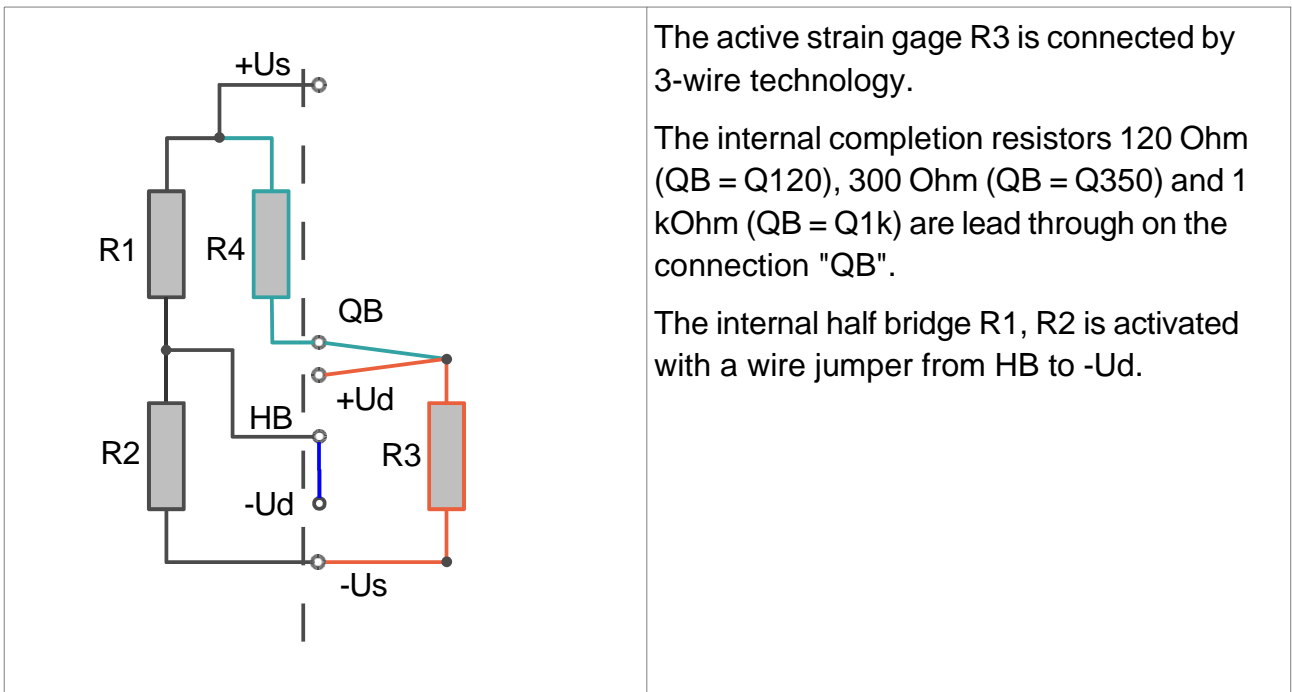

Connection strain gage half bridge

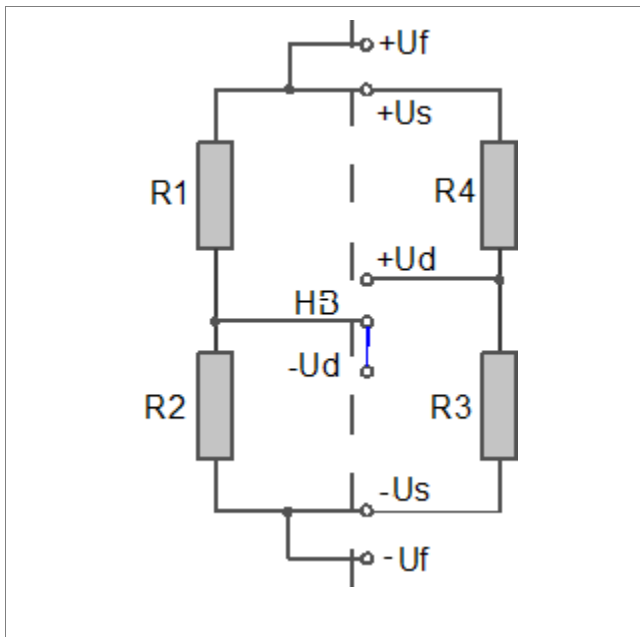


The active strain gages R3 and R4 are connected to +Us, +Ud and -Us.

For very long cable lengths the sense lines +Uf and -Uf can be used.

The internal half bridge R1, R2 is activated with a wire jumper from HB to -Ud.


Connection strain gage full bridge

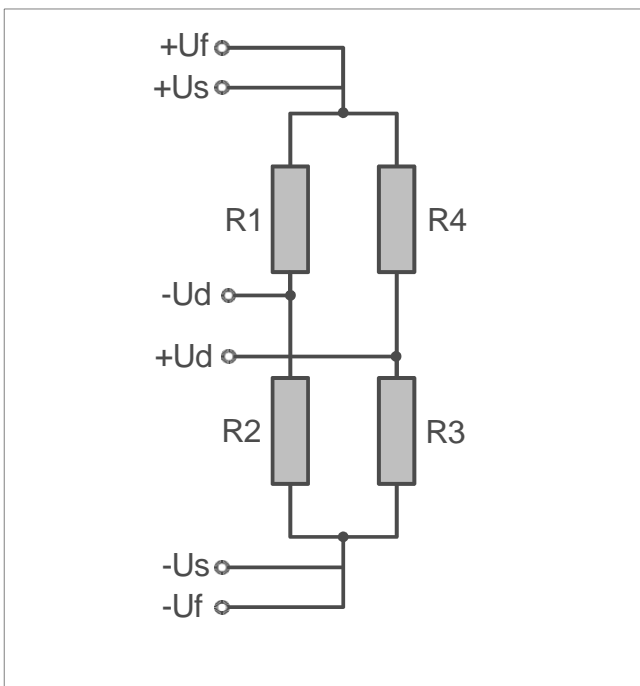

The active strain gages R1 to R4 are connected on +Us,, -Us, +Ud, -Ud.

For very long cable lengths the sense lines +Uf and -Uf can be used additionally (6-wire technology).

Connection of PT1000

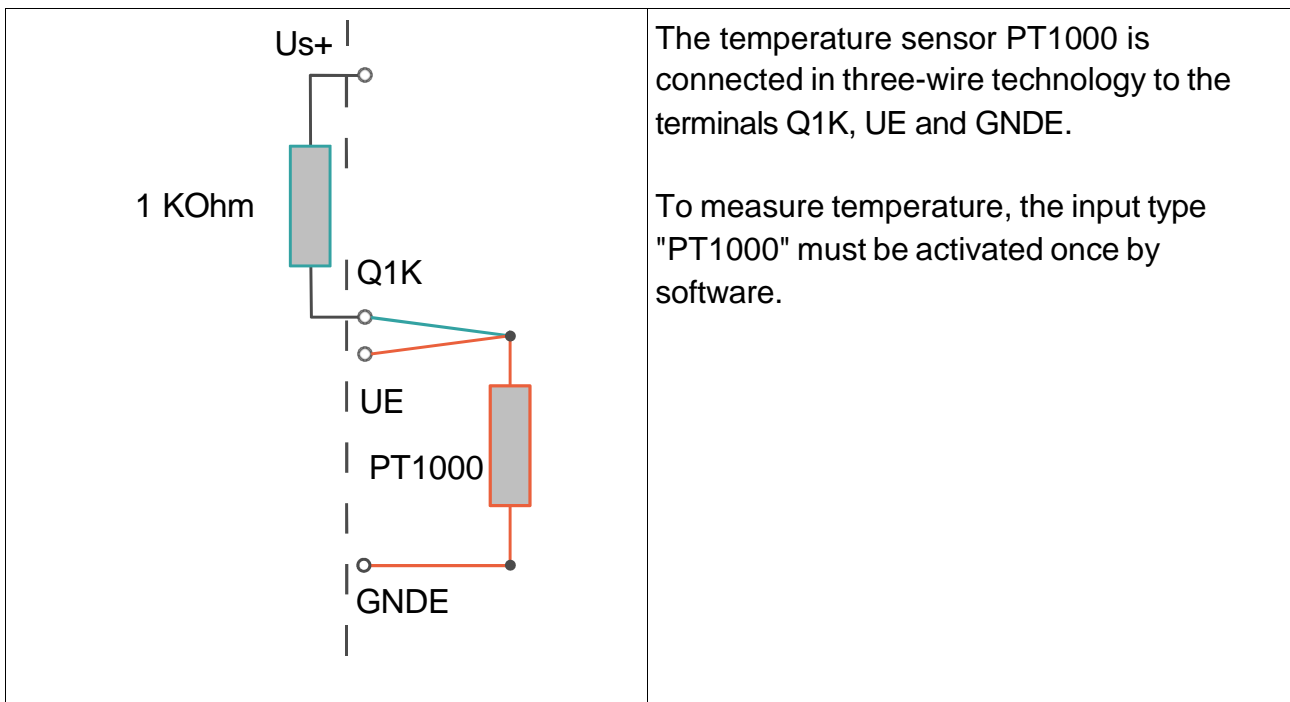

Connection of thermocouple type K

The + wire of the temperature sensor type K is connected to the $+U_d$ input of one of the analog input channels 1 to 7, the - wire to $-U_d$.

To measure the absolute temperature with thermocouple K, a PT1000 reference sensor is required, which must be connected to input channel 8. It should have the same temperature as the type K sensor connector (cold junction compensation).

Relative measurement is also possible with type K; in this case you do not need a reference sensor.

Connection of the active sensors

The single-ended voltage signal of active sensors is applied to U_e and GNDE.


Potentiometric sensors can be supplied via $+U_s$. The energy supply for active sensors can be via galvanic isolated voltage V_{CCIO} and $GNDIO$.

Connection of the TEDS cables for sensors with Transducer Elec. Data sheet

The 1-wire EEPROM memory module located in the sensor or in the sensor connector is connected with two wires: the ground of the EEPROM to GNDE and the signal cable (corresponding to its 3.3V supply cable) at the TEDS connector.

However, TEDS are supported only from firmware version 1.32 on and hardware version 4.0, which are devices that were purchased from about 11/2016.

Analog output 25-pin D-Sub socket

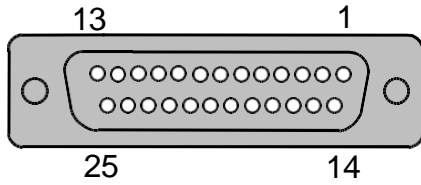


Analog outputs voltage or current for channels 1 to 8.

| Pin | Signal | Meaning |
|-----|----------|------------------------------------|
| 1 | Ua1/ Ia1 | Analog output channel 1 |
| 2 | Ua2/ Ia2 | Analog output channel 2 |
| 3 | Ua3/ Ia3 | Analog output channel 3 |
| 4 | Ua4/ Ia4 | Analog output channel 4 |
| 5 | Ua5/ Ia5 | Analog output channel 5 |
| 6 | Ua6/ Ia6 | Analog output channel 6 |
| 7 | Ua7/ Ia7 | Analog output channel 7 |
| 8 | Ua8/ Ia8 | Analog output channel 8 |
| 9 | / | Internal usage |
| 10 | / | Internal usage |
| 11 | / | Internal usage |
| 12 | OutB- | 60kHz frequency -6V Out (optional) |
| 13 | | Internal usage |
| 14 | GNDA | Analog GND |
| 15 | GNDA | Analog GND |
| 16 | GNDA | Analog GND |
| 17 | GNDA | Analog GND |
| 18 | GNDA | Analog GND |
| 19 | GNDA | Analog GND |
| 20 | GNDA | Analog GND |
| 21 | GNDA | Analog GND |
| 22 | | Internal usage |

| Pin | Signal | Meaning |
|--------|--------|------------------------------------|
| 23 | | Internal usage |
| 24 | OutB+ | 60kHz frequency +6V Out (optional) |
| 25 | GNDINT | GNDINT |
| Shield | PE | Earth (housing) |


Digital in- and outputs 25-pin D-Sub plug connector

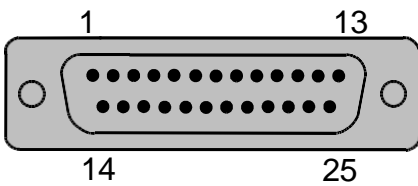

| Pin | Name | Meaning |
|-----|--------|---|
| 1 | VCC | 5V voltage supply, digital |
| 2 | DGND | Digital ground (GND) |
| 3 | DGND | Digital ground (GND) |
| 4 | DGND | Digital ground (GND) |
| 5 | DGND | Digital ground (GND) |
| 6 | DIO 2 | Group 1, 1.2 |
| 7 | DIO 4 | Group 1, 1.4 |
| 8 | DIO 6 | Group 2, 2.2 |
| 9 | DIO 8 | Group 2, 2.4 |
| 10 | DIO 10 | Group 3, 3.2 |
| 11 | DIO 12 | Group 3, 3.4 QEI 1: Encoder input B |
| 12 | DIO 14 | Group 4, 4.2 QEI 2: Encoder / rectangle input A |
| 13 | DIO 16 | Group 4, 4.4 QEI 2: Reset input I |
| 14 | DGND | Digital ground (GND) |
| 15 | DGND | Digital ground (GND) |
| 16 | DGND | Digital ground (GND) |
| 17 | DGND | Digital ground (GND) |
| 18 | DIO 1 | Group 1, 1.1 |


| Pin | Name | Meaning |
|-----|--------|---|
| 19 | DIO 3 | Group 1, 1.3 |
| 20 | DIO 5 | Group 2, 2.1 |
| 21 | DIO 7 | Group 2, 2.3 |
| 22 | DIO 9 | Group 3, 3.1 |
| 23 | DIO 11 | Group 3, 3.3 QEI 1: Encoder / square wave input A |
| 24 | DIO 13 | Group 4, 4.1 QEI 1: Reset / Index Input I |
| 25 | DIO 15 | Group 4, 4.3 QEI 2: Encoder input B |

EtherCat M12 4-pin socket D-coded



| Pin | Name | Meaning |
|--------|------|-----------------|
| 1 | TD+ | Transmit + |
| 2 | RD+ | Receive + |
| 3 | TD- | Transmit - |
| 4 | RD- | Receive - |
| Shield | PE | Earth (housing) |

CANbus M12 5-pin socket / plug A-coded

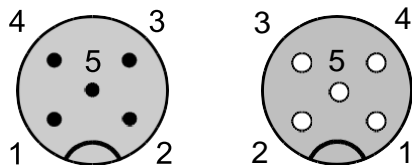


| Pin | Name | Meaning |
|-----|--------|-------------|
| 1 | Shield | Shielding |
| 2 | V+ | Power (UB+) |

| | | |
|---|---------|---------------|
| 3 | V- | GND (0V) |
| 4 | CAN_H | Dominant High |
| 5 | CAN_L | Dominant Low |
| | Housing | Shield |


UART Port 9-pin D-Sub socket

The UART Port may be used for connection of Raspberry PI (3.3V high level) The UART Port is not available for variants "EC" with EtherCat.




| Pin | Name | Meaning |
|-----|---------|--------------------------------------|
| 1 | UB- | Ground supply voltage |
| 2 | RX | Receive data of BX8, 3.3Volt level |
| 3 | TX | Transmit data of BX8, 3.3 Volt level |
| 4 | / | Internal usage |
| 5 | UB- | Ground supply voltage |
| 6 | UB+ | Supply voltage |
| 7 | / | Internal |
| 8 | UB+ | Supply voltage |
| 9 | OFF | BX8 Disable |
| | Housing | Shield |

Voltage supply M8, 4-pin



| | | | |
|---|-----|-------|---------------------------------------|
| 1 | UB+ | brown | Positive supply voltage 10-27V, brown |
| 2 | PE | white | Earth (housing) PE, white |
| 3 | 0V | blue | Negative supply voltage (GND), blue |
| 4 | PE | black | Earth (housing) PE, black |

Screw terminal BX8-AS

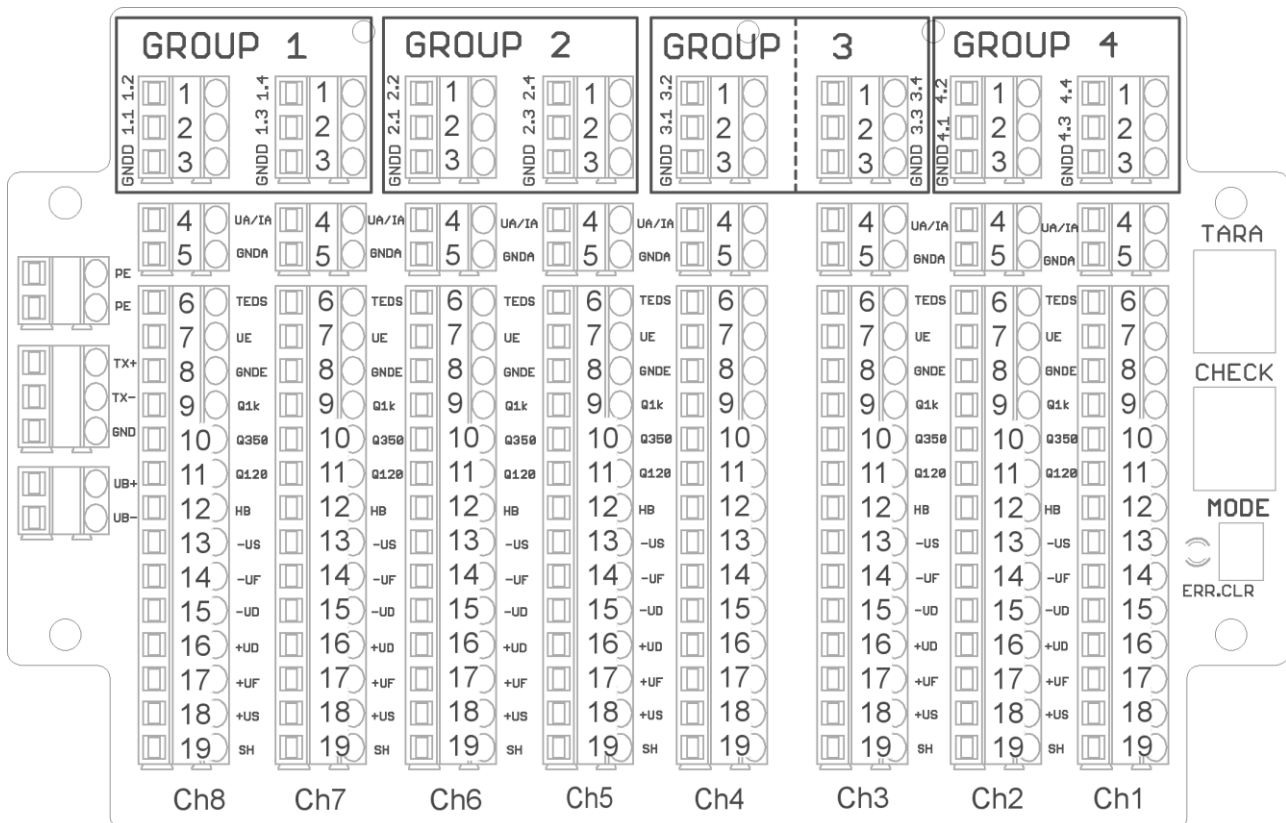

| Pos. | Terminal labelling | Description |
|------|--------------------|--|
| 1 | n.2 / n.4 Group n | Digital In/Out No. 2 / 4 / 6 / 8 / 10 / 12 / 14 / 16 |
| 2 | n.1 / n.3 Group n | Digital In/Out No. 1 / 3 / 5 / 7 / 9 / 11 / 13 / 15 |
| 3 | GNDD | Ground, digital In/Out |
| 4 | UA/IA | Analog output, current or voltage |
| 5 | GNDA | Ground, Analog output |
| 6 | TEDS | Transducer Electronic Data according to IEEE 1451.4 |
| 7 | UE | Voltage, Analog input |

| | | |
|----|------|------------------------------------|
| 8 | GNDE | Ground, Analog input |
| 9 | Q1k | Quarter bridge completion 1000 Ohm |
| 10 | Q350 | Quarter bridge completion 350 Ohm |
| 11 | Q120 | Quarter bridge completion 120 Ohm |
| 12 | HB | Half bridge completion |
| 13 | -US | Negative bridge supply |
| 14 | -UF | Negative sense line |
| 15 | -UD | Negative differential input |
| 16 | +UD | Positive differential input |
| 17 | +UF | Positive sense line |
| 18 | +US | Positive bridge supply |
| 19 | SH | Earth, analog input (shielding) |

Additional information

LED indicators

The LED indicators differ according to the housing versions AS and HD as well as the field bus versions CANopen and Ethercat. The HD housing is equipped with all the LEDs on the front panel, integrated into the buttons. The green ECR or green FUNCTION LED only has significance for Ethercat devices.

| LED | Color AS | Color HD | Meaning | Position AS | Labelling HD |
|----------|----------|----------|-------------------------------|--------------------------|--------------|
| FUNCTION | yellow | blue | on/off, Bootloader | outside, | ON OFF |
| | green | green | Ethercat-State EC-RUN | yellow/green combined | ECR |
| STATUS | red | red | Error state | outside | MOD |
| CHECK | yellow | yellow | Measuring value- emulation | inside | CHK |

For devices with fieldbus (CANopen, Ethercat), there are two small green LEDs next to the field bus connections. These have the following meaning:

Ethercat: Link activity

CANopen: Field bus switched on

LED indicators STATUS and FUNCTION on Ethercat devices

| Device state | FUNCTION-LED | EC-RUN-LED |
|---|-----------------------|-------------------------------------|
| EtherCAT State=INIT (not active) | Permanently on | Off |
| EtherCAT State=PREOP | Off | Blinking 200ms on 200ms off |
| EtherCAT State= SAFEOP | Off | Single flash 200ms on, 1s off |
| EtherCAT State= OP | Off | Permanently on |
| USB-Bootloader active (EtherCAT not used) | 300ms on 300ms off | Off |

LED-display for error condition (all device models)

| Error condition | Prio | STATUS LED | Meaning |
|--|------|--|--|
| EtherCAT: State-transition inhibited | 1 | Blinking 200ms on 200ms off | Requested status transition impossible, e.g. because of invalid settings or invalid hardware settings |
| EtherCAT: State automatically reset | 1 | Single flash 200ms on, 1s off | Device switched from operating state to SafeOpError because of a synchronization error |
| EtherCAT: Application watchdog timeout | 1 | Double flash 200ms on, 200ms off 200ms on 1sec off | If Watchdog-timer is active: process data frame not received within watchdog time |
| Measuring application: Sensor error | 2 | Permanent on | 1. A sensor or its cable is defective, for example, the cable Ud+ or Ud- could be interrupted or could have short circuited with one of the cables Us+ or Us-. 2. A measured value is saturated, i.e., the measuring signal lies outside of the measuring range. This could be ascribed to a defective sensor. 3. The maximum value is exceeded for a six-axis sensor. |
| Measuring application: Error at the digital output | 3 | Blinks slowly 500ms on 500ms off | Short-circuit at the digital output, i.e. if this is connected as an output and switched to High, it has short-circuited with GNDD, or if it is switched to Low, a voltage ≥ 3 V is applied. |
| Measuring application: Error at the analog output | 4 | Blinks very slowly 1s on 1s off | Open current output or overheating of the output driver, for example as a result of a short-circuited voltage output. |
| Bootloader: Firmware-update failed | 1 | Permanent on | Checksum error after writing to flash memory during firmware update |

FUNCTION LED

The FUNCTION LED lights up permanently in yellow (blue for BX8-HD) during normal operation. It blinks after activating the firmware update function (see Annex A).

In EtherCAT devices, this LED lights up or blinks in green depending on the EtherCAT states (with BX8-HD: separate green LED).

STATUS LED (red)

The STATUS LED indicates errors that have occurred.

If it lights up permanently in red, an error at the sensor input has occurred. This can be ascribed to three causes:

- A sensor or its cable is defective, for example, the cable Ud+ or Ud- could be interrupted or short circuited with one of the cables Us+ or Us-.
- A measured value is saturated, i.e. the measuring signal lies outside the measuring range. This could be ascribed to a defective sensor.
- The maximum value is exceeded for a six-axis sensor.

If the STATUS LED blinks slowly (approx. 1x/s), an error has occurred at the analog output. This could be an open current output or overheating of the output driver, for example, as a result of a short-circuited output voltage.

If the STATUS LED blinks quickly (approx. 2x/sec), an error has occurred at the digital output, namely a short circuit, i.e., if this is connected as an output and switched to High, it has short-circuited with GNDD, or if it is switched to Low, a voltage ≥ 3 V is connected.

The status display of the error can be cleared by pressing the MODE button (located in the housing) if the error is currently no longer present.

Detailed error information is stored in the device and can be displayed by pressing the keyboard key E in the terminal program.

Digital inputs and outputs

The BX8 has 16 configurable 5V TTL compatible digital inputs and outputs ('DIOs'). These are organized into 4 groups which are identified on the BX8-AS terminal connections as 'Group 1' to 'Group 4'. The respective DIOs are identified here as <GroupNo.>.<DIONo>.

The DIOs can be configured as an input or output function, whereby the DIOs within one

group must all have the same data direction.

Digital-I/O Numbers

In the devices and windows API (DLL), the numbers of the DIOs are assigned to the terminal connection identification as follows:

| Number in the API and terminal program | Belongs to group | Identification on the terminal board | Assigned optional function / remark |
|--|------------------|--------------------------------------|--|
| 1 | 1 | 1.1 | |
| 2 | 1 | 1.2 | |
| 3 | 1 | 1.3 | |
| 4 | 1 | 1.4 | |
| 5 | 2 | 2.1 | |
| 6 | 2 | 2.2 | |
| 7 | 2 | 2.3 | |
| 8 | 2 | 2.4 | |
| 9 | 3 | 3.1 | Pull-up may be disabled by QEI configuration |
| 10 | 3 | 3.2 | Pull-up may be disabled by QEI configuration |
| 11 | 3 | 3.3 | QEI 1: Pulse input A |
| 12 | 3 | 3.4 | QEI 1: Pulse input A |
| 13 | 4 | 4.1 | Slave-Input or QEI 1: Reset input I |
| 14 | 4 | 4.2 | Slave-Input or QEI 2: Pulse input A |
| 15 | 4 | 4.3 | Slave-Input or QEI 2: Pulse input B |
| 16 | 4 | 4.4 | Slave-Input or QEI 2: Reset input I |

Digital I/O Functions

The following functions can be configured:

| No | Function | Data direction | Parameter Device- or DLL- Command (GSV86)Get/SetDIOType | Short description |
|----|---|----------------|---|---|
| 1 | General-Purpose Input | Input | 0x000004 | General input. The logic level can be queried with GetDIOlevel / GSV86getDIOlevel. |
| 2 | Zero setting single channel | Input | 0x000010 | The active input level sets an analog input channel to zero. |
| 3 | Zero setting all channels | Input | 0x000020 | The active input level sets all analog input channels to zero. |
| 4 | Reset the maximum and minimum value determination | Input | 0x000040 | The active input level resets all maximum and minimum values. |
| 5 | Set the default values of all digital outputs | Input | 0x000050 | Active input level sets all I / Os configured as output to the (configurable) default level. ⁶ |
| 6 | Trigger Send actual value | Input | 0x000080 | Triggers the sending of a measured value frame with actual measured values via a USB interface to the inactive-to-active edge of the digital input. |
| 7 | Trigger minimum value | Input | 0x000100 | The maximum value determination is started for the inactive-to-active edge at the digital input (all input channels) and a frame with these maximum values is sent to the USB interface at the active-to-inactive edge. |
| 8 | Trigger minimum value | Input | 0x000200 | The minimum value determination is started for the inactive-to-active edge at the digital input (all input channels) and a frame with these minimum values is sent to the USB interface at the active-to-inactive edge. |
| 9 | Trigger mean | Input | 0x000400 | A decimating mean value formation is started for |

⁶ Available from firmware-version 1.45

| | | | | |
|----|--|--------|----------|---|
| | value | | | the inactive-to-active edge on the digital input (all input channels) and a frame with these mean values is sent to the USB interface at the active-to-inactive edge. |
| 10 | Trigger Send actual value | Output | 0x000800 | While the input level is active, measured value frames with actual measured values are sent via a USB interface at the set data rate. |
| 11 | Sync-Slave Input | Input | 0x000002 | Input for synchronous measurement data frame transmission in combination with several BX8, whereby the line is connected to the master (see no.20) |
| 12 | QEI-Encoder | Input | 0x000008 | Input for quadrature counter / frequency measurement. Read-Only. To change, the command Write Counter/Freq Mode at Index 0 must be used. ⁷ |
| 13 | General-Purpose Output | Output | 0x001000 | General output. The actual logic level can be defined with SetDIOlevel / GSV86setDIOlevel. |
| 14 | Threshold output actual value | Output | 0x010000 | Threshold value output: The output is activated if the assigned measured value is larger than the upper threshold value and is deactivated if it is smaller than the lower threshold value. |
| 15 | Threshold output maximum value | Output | 0x014000 | Threshold value output: The output is activated if the assigned maximum value is larger than the upper threshold value and is deactivated if it is smaller than the lower threshold value. |
| 16 | Threshold output minimum value | Output | 0x018000 | Threshold value output: The output is activated if the assigned minimum value is larger than the upper threshold value and is deactivated if it is smaller than the lower threshold value. |
| 17 | Window comparator output actual value | Output | 0x012000 | Window comparator: The output is activated if the assigned measured value is smaller than the upper threshold value and larger than the lower threshold value; otherwise it is deactivated. |
| 18 | Window comparator output maximum value | Output | 0x016000 | Window comparator: The output is activated if the assigned maximum value is smaller than the upper threshold value and larger than the lower threshold value; otherwise it is deactivated. |

⁷ Available from firmware-version 1.45

| | | | | |
|----|--|--------|----------|---|
| 19 | Window comparator output minimum value | Output | 0x01A000 | Window comparator: The output is activated if the assigned minimum value is smaller than the upper threshold value and larger than the lower threshold value; otherwise, it is deactivated. |
| 20 | Sync-Master output | Output | 0x020000 | Output to the synchronous data frame transmission in combination with several BX8, whereby the line is connected to the slave(s) (see no.11) |

Inverting digital inputs

The DIOs have pull-up resistances that generate high levels when the input is open. For input trigger functions that are intended to be used with a switch or button, that one must be connected between the DIO and the GNDD terminal. The line must be functionally inverted by software so that the function can be executed when the switch is closed. When using the device interfaces or DLL, the specified value in the above-mentioned column 'Value' must be ORed with 0x80000 for this purpose.

The threshold value outputs can also be inverted in this way. The

terms in the above-mentioned table mean:

| Level | Non-inverted | Inverted |
|----------|---------------------|---------------------|
| Active | Logic 1 = High = 5V | Logic 0 = Low = 0V |
| Inactive | Logic 0 = Low = 0V | Logic 1 = High = 5V |

When using the general-purpose functions or the Value-frame sync. functions (no. 1, 11, 13 and 20 in the above table) the inversion has no effect. The software functions/device commands GSV86get/setDIOlevel and Get/SetDIOlevel always read the level directly, i.e. not inverted.

Further Notes Digital I/O

The default level can be defined for digital outputs, i.e., the level that the output should take after restarting and after a reconfiguration. This setting also applies directly, i.e., independent of the inversion state.

The general permanent data transmission should be turned off for measured value-send- trigger functions (no. 6 to 10 in the above-mentioned table). This can be done with the button in the terminal program.

For functions, that are associated with the acquisition of maximum and minimum values (in the table above no. 4,7,8,15,16,18,19) the determination of maximum and minimum values of the firmware should be activated. This can be done with the button m in the terminal program.

Master-Slave Frame Synchronization

When using several BX8s at the same time, the transmission of the measurement data frames can be synchronized via digital I / Os. For this, one of the devices must be configured as a master by selecting one of the DIO lines as a synchronization line and configuring the function of this line as a sync master output (no.20). All other devices are configured as sync slave input (No. 2) on one of the DIO lines 13 to 16, that are connected to the master.

When using the optional BX8 master-slave adapter cable, the synchronization line for all devices is set to DIO no. 16.

The synchronization line always consists of two wires: signal (e.g., DIO 16 <-> DIO 16) and GND = digital reference mass.

Counter, frequency, and speed measurement

Devices with firmware version 1.45 and following can also evaluate data of incremental encoders, such as rotary encoder sensors ("QE1"). Up to two quadrature encoders can be connected, each with A, B and optional reset input I, see Digital Inputs Sub-D25 connector. The 6 connection lines have a fixed assignment to the I/O lines: QE1 1: DIO11 to 13. QE1 2: DIO 14 to 16. Likewise, pulses of digital square wave signals can be counted, e.g., for rotation angle or distance measurements. In this case, the input A is the pulse input and B determines the counting direction. Also, the frequency and the quantities associated with it (e.g., translatory motion or rotational speed) can be acquired by the BX8, and the sign of the measured value thereby indicates the direction.

For this purpose, one to two separate measuring channels are used, which are only available after activation of the function. These are always the last two measurement channels in the measurement data frame, or only the last one. As a result, up to 10 measuring channels can be transmitted.

The first encoder "QE1 1" can be used to measure counter, frequency or both counter and frequency / speed at the same time. In the latter case, two measurement channels are generated.

Encoders which generate single-ended square wave signals having the states 0V (connected to GND) and 5V, or 0V and high impedance, i.e., 5V TTL push-pull outputs or open drain, can be connected directly. A power supply with 5V and max. 20mA is available. The maximum input frequency is 10 MHz.

Details on configuration and mode of operation are described in a separate document "BA- BX8-Incrementalencoder_en.pdf".

Data Acquisition and Bandwidth

The BX8 has a 24-bit sigma delta AD converter that acquires all 8 channels simultaneously (simultaneous sampling). It is set to a fixed single sampling rate of 48000 samples/second (total sampling rate = 48000/s x 8 channels = 384000/s). These are decimated down by a digital anti-aliasing filter to fixed values depending on the selected data rate, whereby all input samples are included in the calculation (output decimation).

The cut-off frequencies mentioned in the following table is a result of this input filter, i.e. these apply if:

- The analog input filter is set to the highest value of 11.4 kHz and

In this case, the data frequency also automatically corresponds to the update of the analog output. However, the analog output is updated up to 16000 samples / s. The analog output is switched off from 24000 samples / s and higher.

- The additional digital filters (see above) are switched off.

| Data frequency in frames/s | Decimation divisor | -3 dB cut-off frequency in Hz |
|----------------------------|--------------------|-------------------------------|
| 1 | 48000 | 0,4 |
| 2 | 24000 | 0,8 |
| 3 | 16000 | 1,2 |
| 4 | 12000 | 1,6 |
| 5 | 9600 | 2 |
| 6 | 8000 | 2,4 |
| 8 | 6000 | 3,2 |
| 10 | 4800 | 4 |
| 12 | 4000 | 4,8 |
| 15 | 3200 | 6 |
| 16 | 3000 | 6,4 |
| 20 | 2400 | 8 |
| 24 | 2000 | 9,6 |
| 25 | 1920 | 10 |
| 30 | 1600 | 12 |
| 32 | 1500 | 12,8 |

| Data frequency in frames/s | Decimation divisor | -3 dB cut-off frequency in Hz |
|----------------------------|--------------------|-------------------------------|
| 40 | 1200 | 16 |
| 48 | 1000 | 19,2 |
| 50 | 960 | 20 |
| 60 | 800 | 24 |
| 75 | 640 | 30 |
| 80 | 600 | 32 |
| 96 | 500 | 38,4 |
| 100 | 480 | 40 |
| 120 | 400 | 48 |
| 125 | 384 | 50 |
| 150 | 320 | 60 |
| 160 | 300 | 64 |
| 192 | 250 | 76,8 |
| 200 | 240 | 80 |
| 240 | 200 | 96 |
| 250 | 192 | 100 |
| 300 | 160 | 120 |
| 320 | 150 | 128 |
| 375 | 128 | 150 |
| 384 | 125 | 153,6 |
| 400 | 120 | 160 |
| 480 | 100 | 192 |
| 500 | 96 | 200 |
| 600 | 80 | 240 |
| 640 | 75 | 256 |
| 750 | 64 | 300 |
| 800 | 60 | 320 |
| 960 | 50 | 384 |
| 1000 | 48 | 400 |

| Data frequency in frames/s | Decimation divisor | -3 dB cut-off frequency in Hz |
|----------------------------|--------------------|-------------------------------|
| 1200 | 40 | 480 |
| 1500 | 32 | 600 |
| 1600 | 30 | 640 |
| 1920 | 25 | 768 |
| 2000 | 24 | 800 |
| 2400 | 20 | 960 |
| 3000 | 16 | 1200 |
| 3200 | 15 | 1280 |
| 4000 | 12 | 1600 |
| 4800 | 10 | 1920 |
| 6000 | 8 | 2400 |
| 8000 | 6 | 3200 |
| 9600 | 5 | 3840 |
| 12000 | 4 | 4800 |
| 16000 | 3 | 6400 |
| 24000 | 2 | 9600 |
| 48000 | 1 | 11400 |

Note: The configurable maximum data frequency depends on other settings of the device.

When setting the data frequency, the BX8 checks if the desired data frequency is possible and refuses the command, if not. The maximum configurable data frequency can be determined by a read command. Examples of settings that have an impact on the maximum data frequency, are:

- Measured data type
- Bit rate of the UART interface, if activated (if present)
- Digital FIR- and IIR-filters
- Trigger- and threshold functions of the digital I/Os
- Activated six-axis sensor measuring

At the highest data rates of 24000 / s and 48000 / s, the range of functions of the BX8 is limited to digital data transmission.

Data frames and data throughput

The BX8 transmits the measured data in single frames via a serial USB interface, whereby

each measured data frame contains samples of all 8 channels that were acquired simultaneously.

The data format for the measured data can be changed. There are 3 different data formats available:

| Data type | Description | Maximum data frequency ⁸ |
|-----------|--|--|
| INT16 | Integer 16-Bit-value in binary offset format. Unscaled raw value. | 48000 frames/s |
| INT24 | Integer 24-Bit-value in binary offset format. Unscaled raw value. | 24000 frames/s |
| Float | 32-bit floating-point number according to IEEE 754. Measured value has been completely scaled. | 12000 frames/s (six-axis sensor = off) ⁹ 12000 frames/s (six-axis sensor = on) ¹⁰ |

Using the example of the strain gage input with a bridge supply voltage of 8.75 V, the following applies for the integer measured value display INT16 and INT24:

| Sensor deviation in mV/V | Integer measuring value, 16-Bit Hex | Integer measuring value, 24-Bit Hex | Read value MEGSV8w32.dll: GSVread and other measuring value -read functions ¹¹ |
|--------------------------|-------------------------------------|-------------------------------------|---|
| <= -2,1 | 0x0000 | 0x000000 | -1,05 |
| -2,0 | 0x0618 | 0x061862 | -1,0 |
| 0 | 0x8000 | 0x800000 | 0,0 |
| 2,0 | 0xF9E7 | 0xF9E79E | 1,0 |
| >= 2,1 | 0xFFFF | 0xFFFFF | 1,05 |

The measuring amplifier is factory-calibrated so that the value for the nominal input sensitivity (here 2.0 mV/V) is as exact as possible.

The multiplication with the scaling value (button 'n' in the terminal program) is carried out by external software for the INT data types.

The BX8 independently calculates the completely scaled measured values for the data type float either by taking the scaling value (general sensors) into consideration or by multiplying with the coefficient matrix for the activated six-axis sensors or by using the calculation for PT1000 RTDs.

⁸ This value may be smaller depending on configuration. The BX8 rejects an attempt to set a data frequency that is too high.

⁹ from Firmware 1.36 and higher

¹⁰ from Firmware 1.36 and higher

¹¹ This value doesn't apply for the BX8, if the configured data type is float.

Analog outputs

The signals of the 8 analog correspond to the 8 analog inputs¹², but their signal conforms to that of the digital communication interfaces, so configurations such as physical values of the 6-axis sensors and digital filters also apply to the analog outputs. The maximum value given by the configuration (e.g., + 3.5mV / V or maximum value of the 6-axis sensor) corresponds to the maximum value of the output signal (e.g., + 10V or 20mA). This relation can be reconfigured by individual scaling values for each analog output, also the zero point can be adjusted. The following 5 output types can be configured individually for each channel:

Voltage: 0-10V, ± 10V, 0-5V, ± 5V, current: 4-20mA, 0-20mA

Transducer Electronic Data Sheet according to IEEE1451.4 (TEDS)

The BX8 can be configured to automatically read and use sensors with TEDS memory that contain (currently) TEDS 33 (Bridge Sensor) or 35 (Strain Gage) data , The value of the user scaling is adjusted based on the TEDS data. The setting whether TEDS data is to be used or not is individually configurable for each of the 8 input channels. It is also possible to set whether the unit and the input measuring range should also be adjusted automatically. The previously manually set values of these parameters remain stored in the BX8; if the TEDS sensor is no longer connected, it will be restored.

With the BX8, the recalibration of a TEDS sensor with templates 33 or 35 can also be stored in it, he is TEDS writeable.

Frequency output 60kHz ±30khz (devices option)

The measuring signal of the channel 1 can be additionally represented as a frequency modulated square wave signal. It is a differential signal with an amplitude of 6Vpp. The signal can be picked up on the terminals Tx+, Tx- and GND.

The connection on GND is optional.

The representation of sensor zero signal is with 60kHz. At maximum positive nominal input detuning of the amplifier the frequency increases to 90kHz. At maximum negative nominal input detuning of the amplifier the frequency sinks to 30kHz.

A user scaling value can be supplied which allows for changing the output scaling.

The total range of the frequency output, however, is set to 28500Hz to 91500Hz (30000-5% from the hub to 90,000 + 5%).

¹² From firmware version 1.46, output channel 7 and 8 can be assigned to one of the counter/frequency channels. However, the assignment to analog input 7 and 8 remains in delivery state.

Warranty

All instrument products from Interface Inc., ('Interface') are warranted against defective material and workmanship for a period of (1) one year from the date of dispatch. If the 'Interface' product you purchase appears to have a defect in material or workmanship or fails during normal use within the period, please contact your Distributor, who will assist you in resolving the problem. If it is necessary to return the product to 'Interface' please include a note stating name, company, address, phone number and a detailed description of the problem. Also, please indicate if it is a warranty repair. The sender is responsible for shipping charges, freight insurance and proper packaging to prevent breakage in transit. 'Interface' warranty does not apply to defects resulting from action of the buyer such as mishandling, improper interfacing, operation outside of design limits, improper repair or unauthorized modification. No other warranties are expressed or implied. 'Interface' specifically disclaims any implied warranties of merchantability or fitness for a specific purpose. The remedies outlined above are the buyer's only remedies. 'Interface' will not be liable for direct, indirect, special, incidental or consequential damages whether based on the contract, tort or other legal theory. Any corrective maintenance required after the warranty period should be performed by 'Interface' approved personnel only.